

FIG. 1

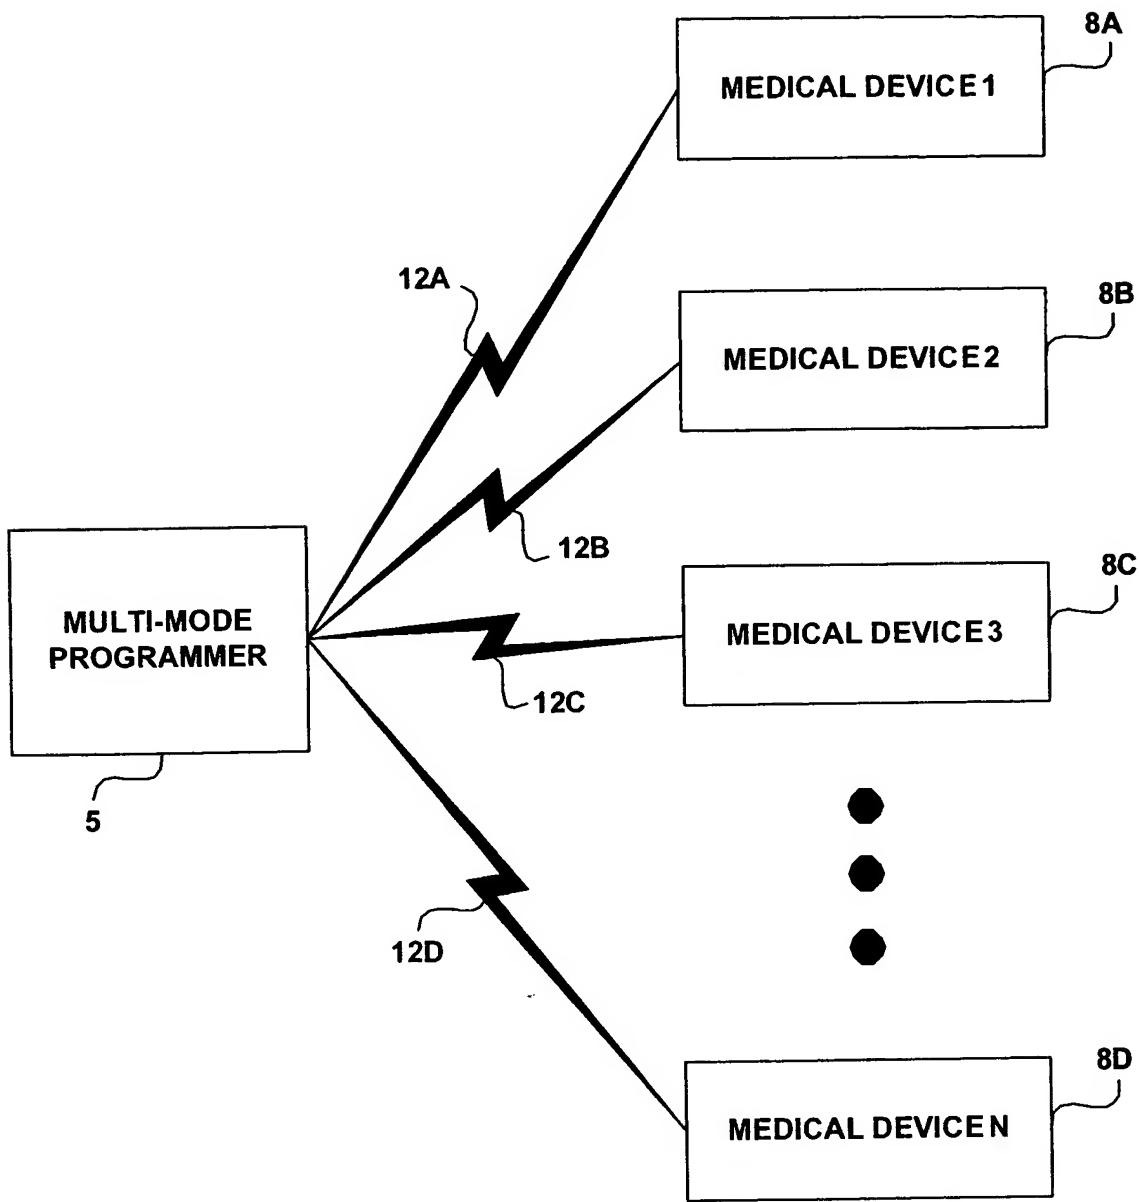


FIG. 2

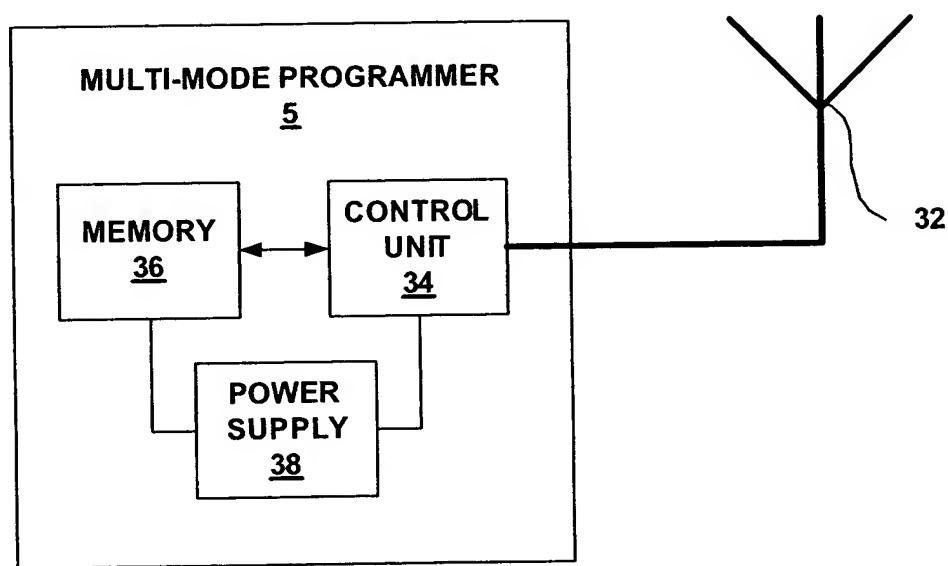


FIG. 3

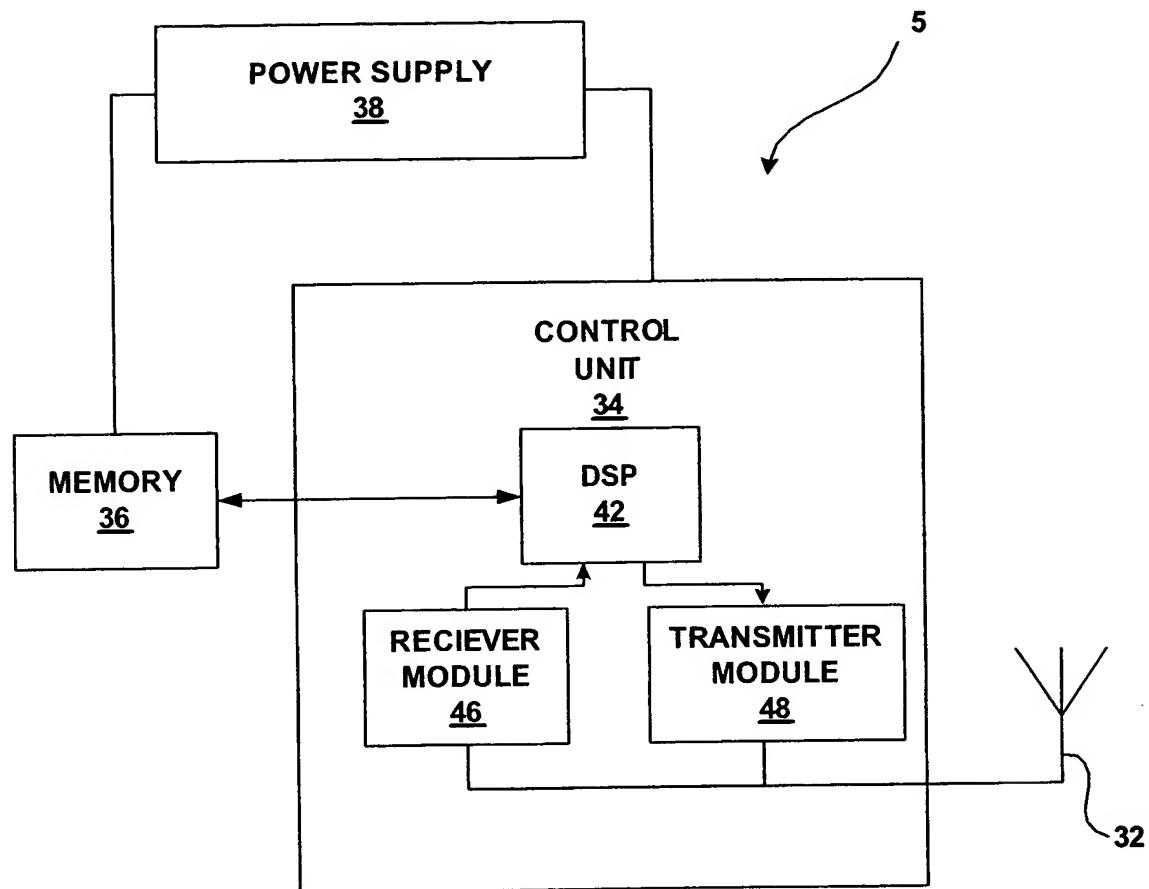


FIG. 4

APPLICANT: GREENINGER ET AL.
TITLE: MULTI-MODE PROGRAMMER FOR MEDICAL DEVICE COMMUNICATION
ATTORNEY/AGENT: GIRMA WOLDE-MICHAEL
REG. NO. 36,724 TELEPHONE: 763.514.6402
DOCKET NO.: P-10520.00 SHEET 5 OF 7

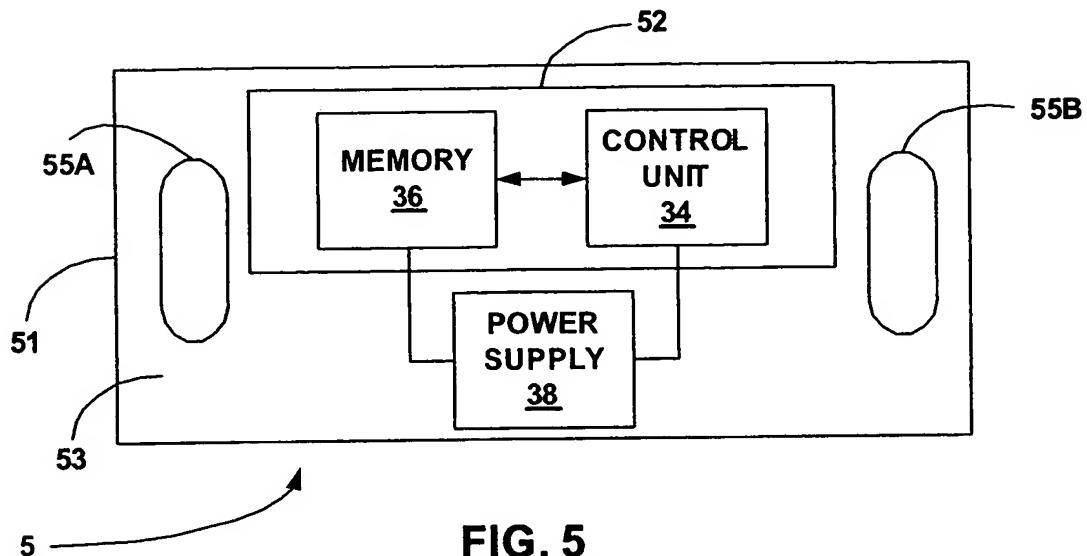


FIG. 5

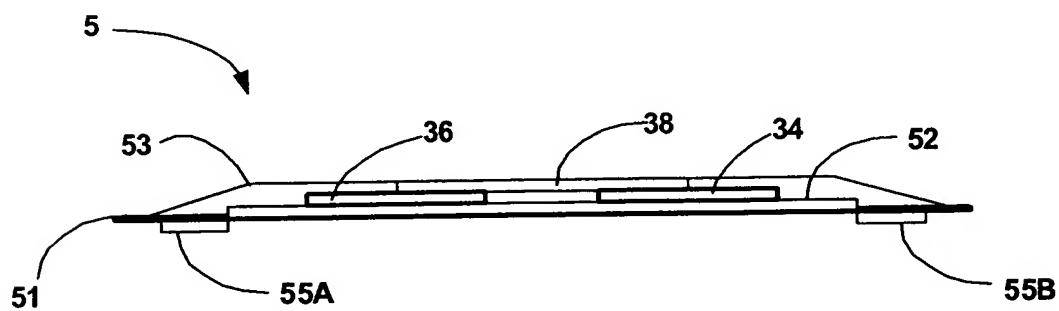


FIG. 6

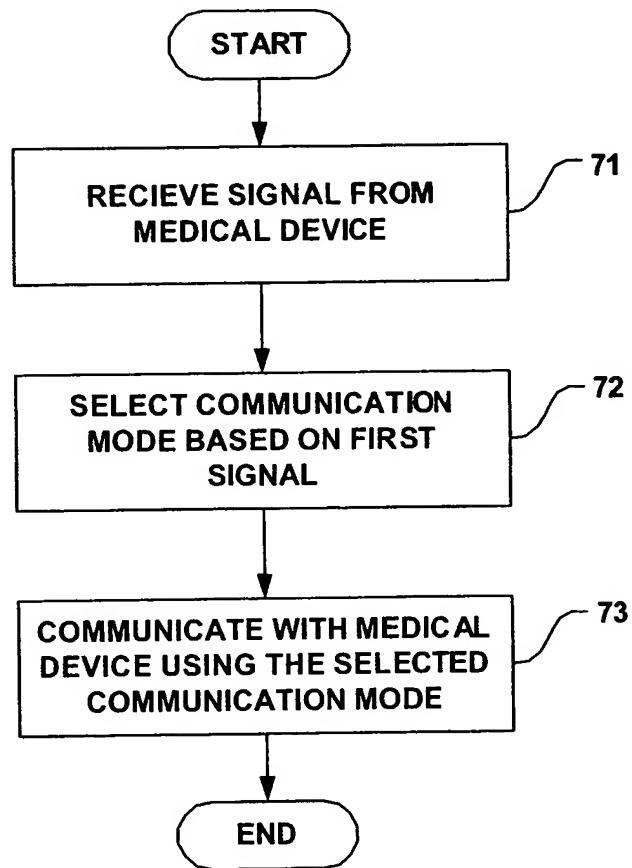


FIG. 7

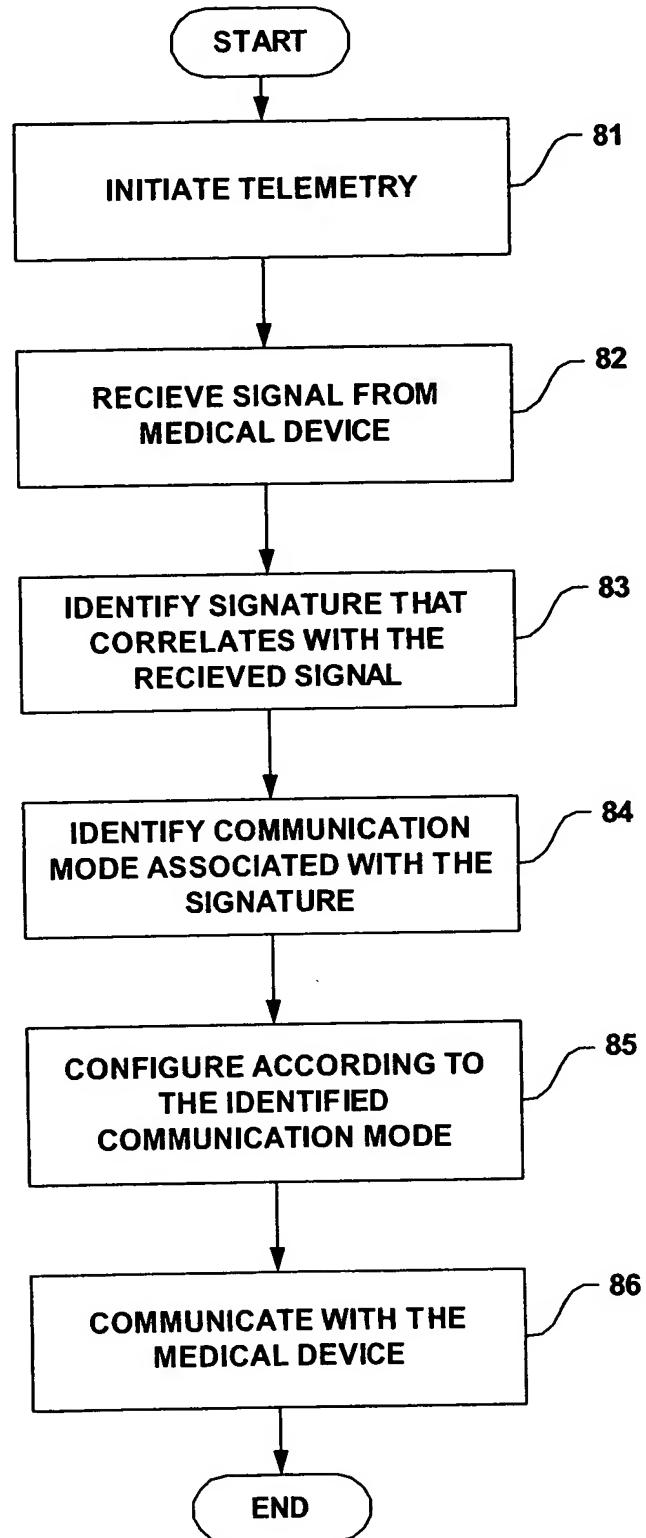


FIG. 8

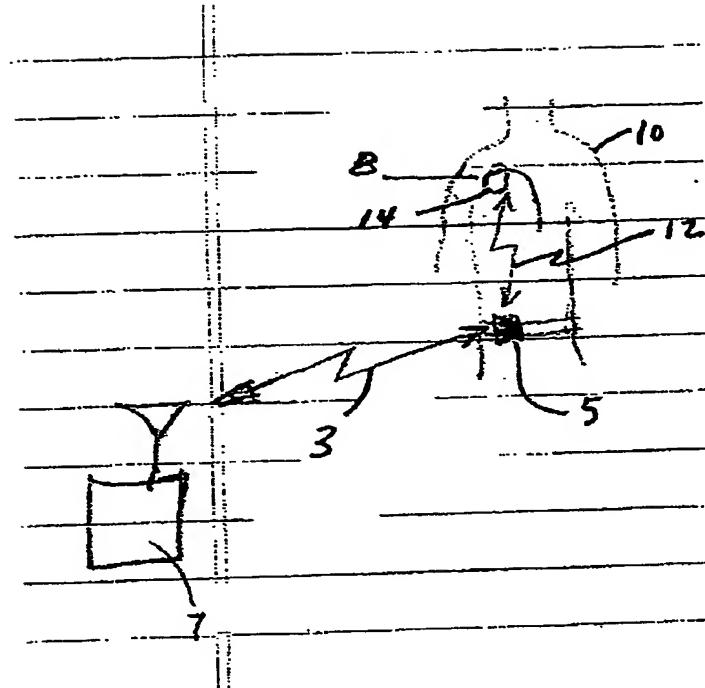


FIGURE 9

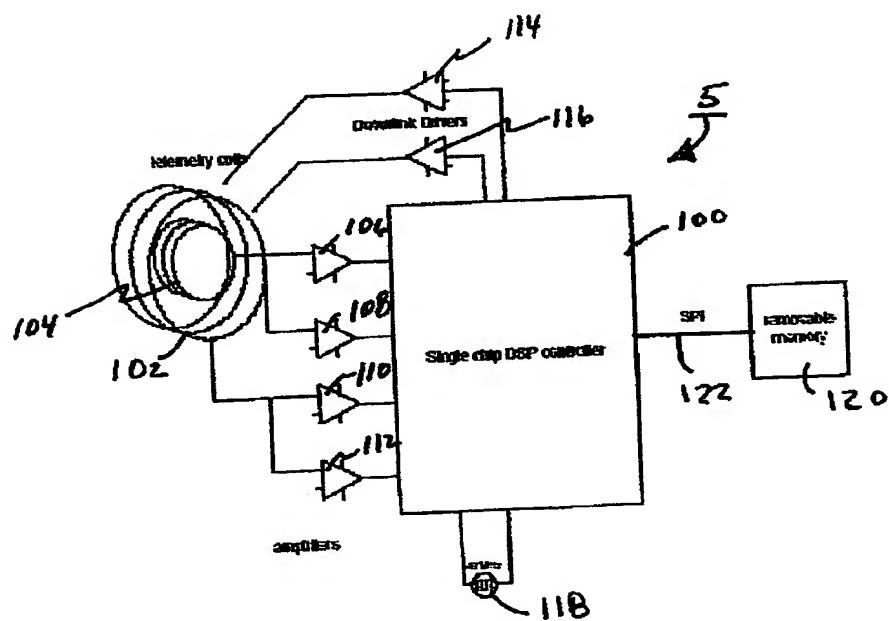


FIG 10

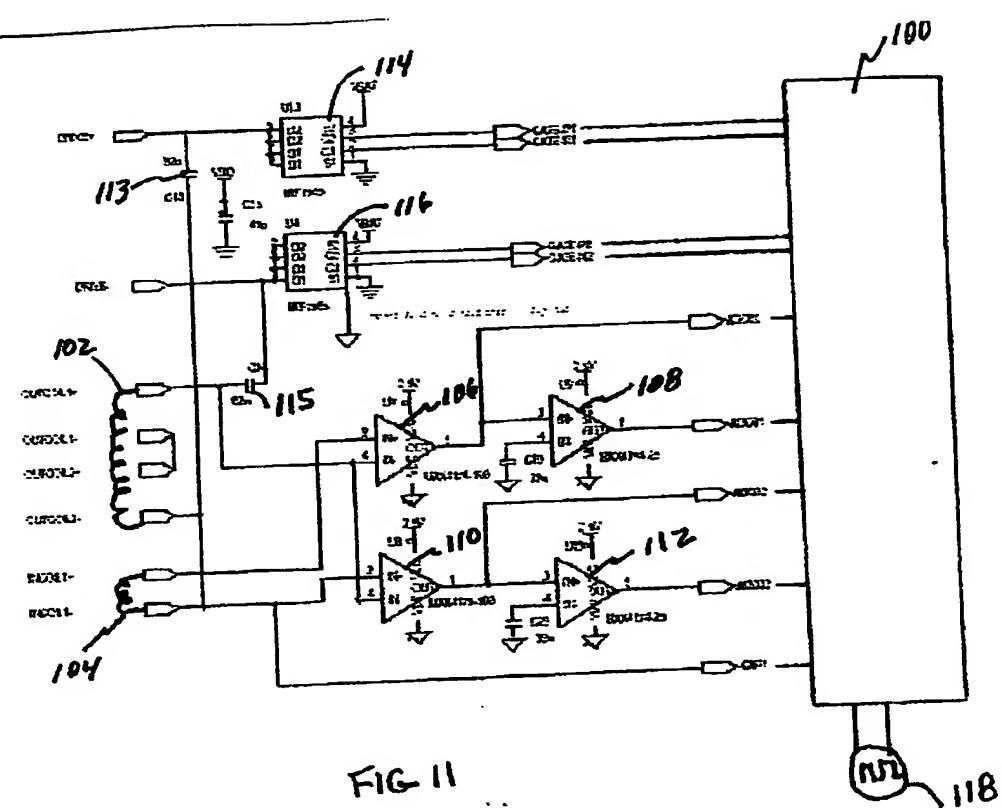


FIG-11

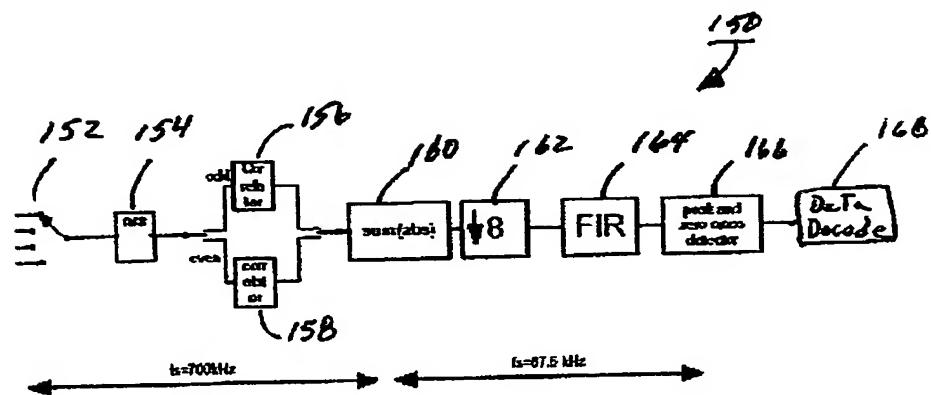


FIGURE 12

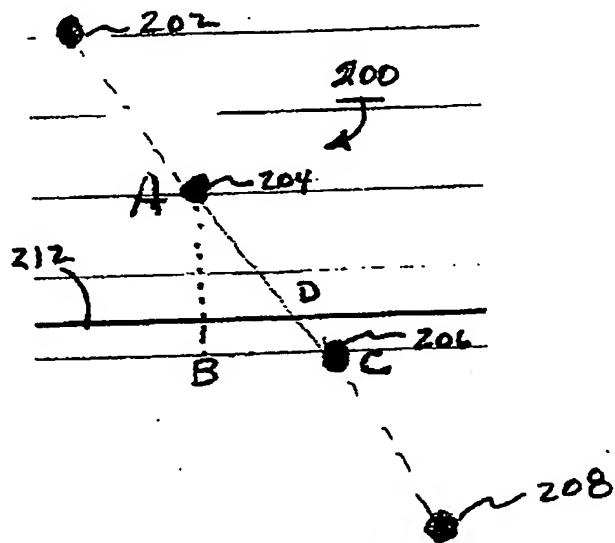


FIGURE 13

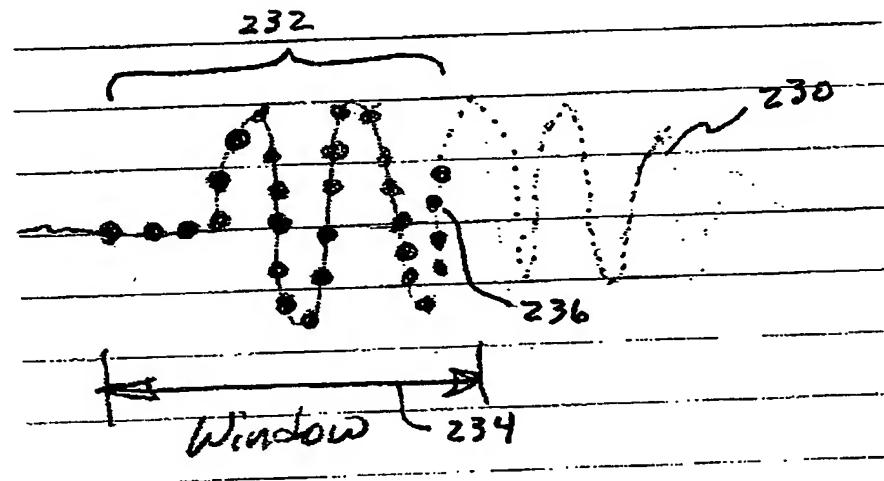


FIGURE 14